

The modified inductance element La

I – INTRODUCTION

It is convenient to use a Constant Phase Element (CPE) instead of a capacitor when for instance the Nyquist diagram of the impedance of a system shows a semi-circle whose center is located below the Real axis, instead of on the Real axis.

The difference between a capacitor C and a CPE Q is that the expression of the impedance of a CPE contains an additional parameter α :

$$Z_Q(f) = \frac{1}{Q(j2\pi f)^\alpha} \quad (1)$$

whereas the expression of the impedance of the capacitor is :

$$Z_C(f) = \frac{1}{C(j2\pi f)} \quad (2)$$

with C and Q the value of the capacitor in F and of the CPE in $F s^{(\alpha-1)}$ with $0 < \alpha \leq 1$. It is important to note that $Z(f)_Q = Z(f)_C$ for $\alpha = 1$. A CPE is physically interpreted as an effect of the surface roughness of the sample, leading to an heterogeneity of the capacitance.

Analogously, the modified inductance La can be used to represent the presence of an unusual inductance in the Nyquist diagram. The expression of the impedance of an inductance is :

$$Z_L(f) = Lj2\pi f \quad (3)$$

The expression of the impedance of the modified inductance La is :

$$Z_{La}(f) = L_a(j2\pi f)^\alpha \quad (4)$$

with L and La the value of the inductance in H and of the modified inductance in $H s^{(\alpha-1)}$,

respectively, with $0 < \alpha \leq 1$. Again, $Z_{La}(f) = Z_L(f)$ for $\alpha = 1$.

This application note introduces a few practical examples for which the modified inductance component can lead to a much better fit of impedance data.

II – HIGH-FREQUENCY INDUCTANCE IN LI-ION BATTERIES

Figure 1 shows the Nyquist impedance diagram of an LiPF₆ Li-ion battery with a capacity of 60 Ah and a nominal voltage of 3.2 V. An inductive behaviour can be seen at high frequencies ($f > 22$ Hz), most likely due to the connection cables to the battery. This behaviour is more visible in cells with low apparent resistance such as batteries. As shown by the least square linear fit in Fig. 1, these high frequency data points are on a straight line that is not perpendicular to the x-axis. Consequently, this behaviour cannot be represented by a simple inductance.

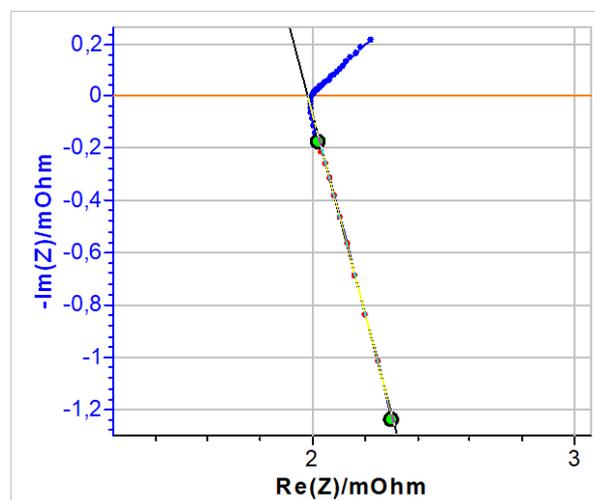


Figure 1 : Nyquist impedance diagram of an LiPF₆ battery for frequencies $\in [0.1, 2000]$ Hz.

Figure 2 shows the equivalent circuit chosen to fit the data shown in Fig. 1.

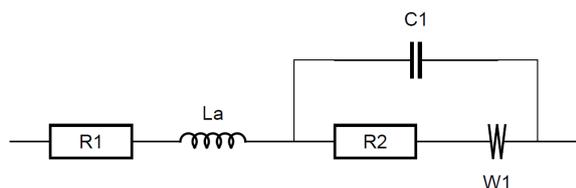


Figure 2 : Randles equivalent circuit with a modified inductance in series.

It is a Randles circuit with an inductance L_a in series. The simple L is a particular example of the inductance L_a . As stated above, if $a=1$, $L_a \equiv L$. R_1 is associated to the internal resistance of the battery, C_1 to the double layer capacitance, R_2 to the charge transfer resistance and W , the Warburg component, to the semi-infinite diffusion.

Figure 3 shows the fitting curve obtained using the equivalent circuit shown in Fig. 2 with a simple inductance. Fig. 4 shows the same results but with a modified inductance L_a . A comparison of the results of the two fitting, *i.e.* the values of the parameters and of χ^2 (an estimation of the goodness of the fit [1]) are given in Table 1.

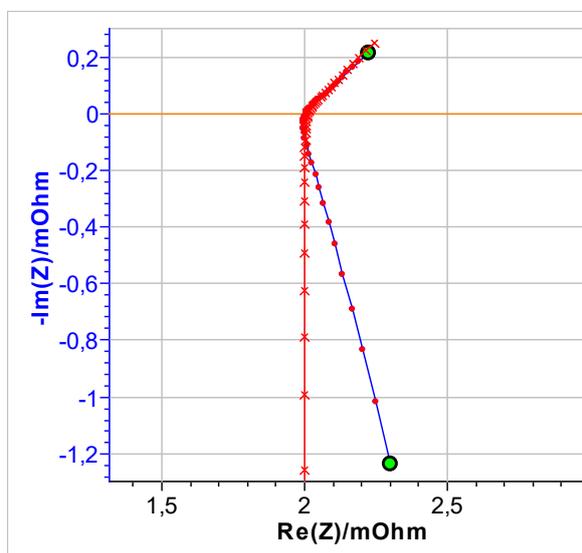


Figure 3 : Fitting results of the impedance diagram in Fig. 1 using the equivalent circuit : $L_1+R_1+C_1/(R_2+W_1)$.

If, instead of an inductance L , a modified inductance L_a is used as shown in Fig. 3, it is possible to fit the non-vertical high frequency part of the impedance. Fig. 4 shows the results

of the fitting of the battery impedance in Fig. 1 using the modified inductance in series with a Randles equivalent circuit. In this case, χ^2 is lower and hence better than the χ^2 factor obtained with an equivalent circuit containing a simple inductance (cf. Table 1). Furthermore, in Table I, it can be seen that the values of C_1 , R_2 and W_1 are different, which shows that using a modified inductance leads to a better determination of the characteristic parameters of the system.

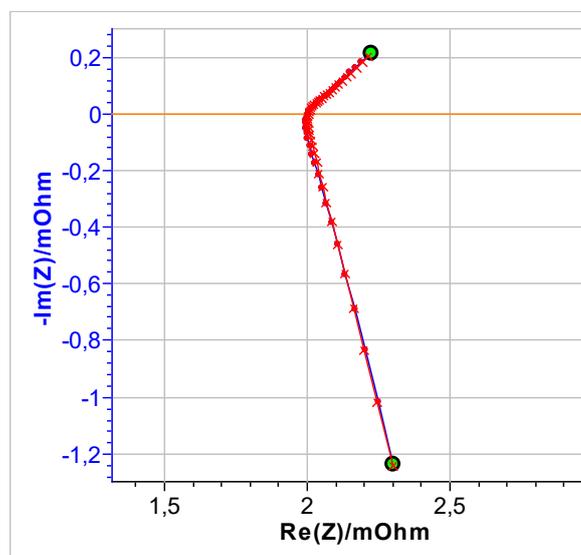


Figure 4 : Fitting results of the graph in Fig. 1 using the equivalent circuit : $L_{a1}+R_1+C_1/(R_2+W_1)$.

Table I : Values of the parameters for the equivalent circuits used in Fig. 3 and Fig. 4.

Parameter	Using L (Fig. 3)	Using L_a (Fig. 4)
$L_1 / \mu\text{Hs}^{(a-1)}$	0.14	0.48
a_1	1	0.84
$R_1 / \text{m}\Omega$	2	2
C_1 / F	109	429
$R_2 / \mu\Omega$	14.3	50.3
$s_1 / \text{m}\Omega \text{ s}^{-1/2}$	0.17	0.158
χ^2	0.53×10^{-6}	2.67×10^{-9}

III – LOW FREQUENCY INDUCTIVE BEHAVIOR OF A FREELY CORRODING METAL

Another example of a system for which the component L_a can be used is a metal corroding in an acidic solution. In this case, the reduction reaction is the proton reduction,

which involves an adsorption step, following the Volmer-Heyrovský mechanism [2, 3]. Fig. 5 shows the impedance graph obtained on a partially painted Zn sample immersed in 0.5 mol L⁻¹ H₂SO₄ and the corresponding fitting curve using the equivalent circuit shown in Fig. 6.

In this equivalent circuit, Q1/R1 is associated to the larger semi-circle in Fig. 5 (possibly related to the coated part of the sample), Q2/R2 to the inductive semi-circle (related to an adsorption process at the rough metal surface) and Q3/R3 to the third semi-circle (also possibly related to the bare metal). The solution used in this example was not a perfect ionic conductor but its resistance of around 1 Ω was considered negligible.

Another way to interpret the impedance diagram is to consider a Volmer-Heyrovský chemical desorption mechanism.

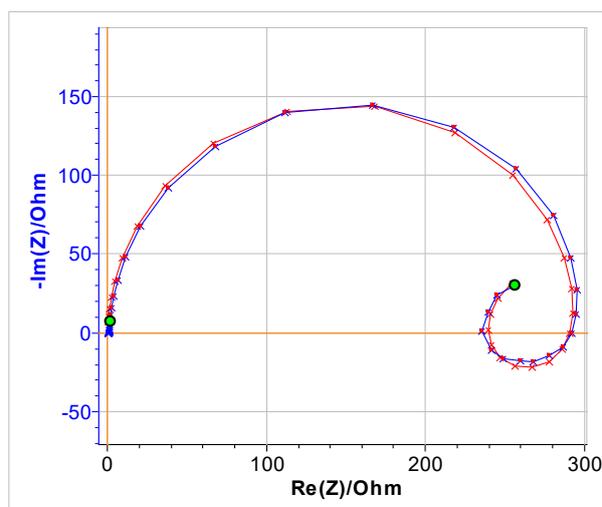


Figure 5 : **Blue :** Nyquist diagram of the impedance of a partially coated Zn sample immersed in 0.5 mol L⁻¹ H₂SO₄ for frequencies $\in [10 \times 10^{-3}, 200 \times 10^3]$ Hz.
Red : Fitting curve using Q1/(R1+Q2/R2+Q3/R3).

In the fitting results shown in Table II, the elements Q2/R2 correspond to the inductive loop and have negative values. It might be difficult for the user to handle and interpret negative values. It is then possible to use an equivalent circuit for which the elements have positive values. This can be done by replacing

the circuit R1+Q2/R2 in Fig. 6 by R1/(R2+La2) as shown in Fig. 7.

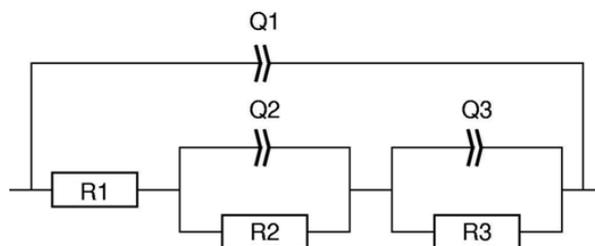


Figure 6: Equivalent circuit used in Fig. 5.

Table II : Values of the parameters for the equivalent circuits used in Fig. 5.

Parameter	Fig. 5 Red
Q1 /μF s ^(a-1)	65.5
a1	0.982
R1 /Ω	298
Q2 /F s ^(a-1)	-0.015
a2	0.907
R2 /Ω	-75.1
Q3 /F s ^(a-1)	0.168
a3	0.826
R3 /Ω	122
χ ²	325

In Fig. 8, the **blue** curve shows the experimental data, the **red** curve, the fitting curve obtained using the equivalent circuit in Fig. 7 with a simple inductance (a2 = 1) and the **green** curve, the fitting curve obtained using the equivalent circuit in Fig. 7 with a modified inductance.

As can be seen in Table III, all the elements of the equivalent circuit have now positive values. In terms of choosing the best equivalent circuit, it seems the **red** curve fit less tightly to the real data than the **green** curve, which shows that the modified inductance increases the goodness of the fit (see

inset of Fig. 8). This is confirmed by the values of the χ^2 shown in Table 3.

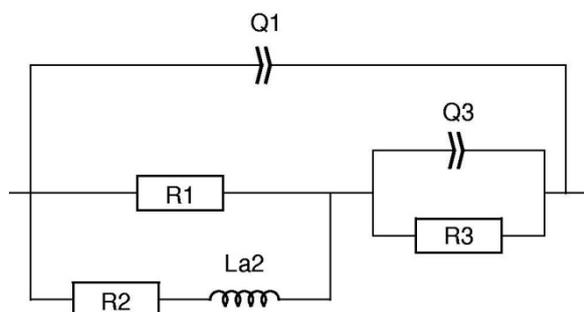


Figure 7: Equivalent circuit used in Fig. 8.

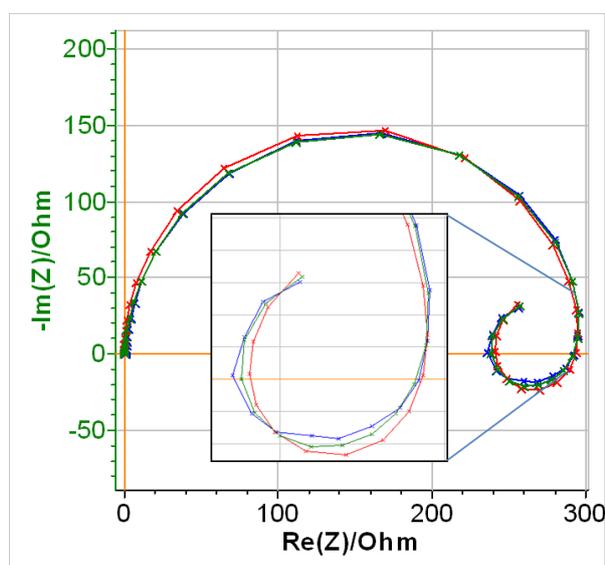


Figure 8: **Blue** : Nyquist diagram of the impedance of a partially coated Zn sample immersed in 0.5 mol L⁻¹ H₂SO₄. Fitting curve using **Red** : Q1/(R1/(R2+L2)+Q3/R3), **Green** : Q1/(R1/(R2+La2)+Q3/R3).

Table III : Values of the parameters for the equivalent circuits used in Fig. 8.

Parameter	Using L Fig. 8 Red	Using La Fig. 8 Green
Q1 / $\mu\text{F s}^{(a-1)}$	65.9	74
a1	0.981	0.958
R1 / Ω	299	313
L2 /H s ^(a-1)	1464	837
a2	1	0.645
R2 / Ω	1118	1.33 x10 ⁻⁹
Q3 /F s ^(a-1)	0.348	0.020
a3	1	0.718
R3 / Ω	87.5	325
χ^2	277	60

IV – CONCLUSION

The new element La is a modified inductance element. It can be used to fit impedance characteristics related to either an unusual connection inductance at high frequencies, mostly visible in batteries or a heterogeneous adsorption mechanism at low frequencies, mostly visible in corrosion.

REFERENCES

- 1) EC-Lab® User's Manual p. 113
- 2) M. Keddam, Thèse, Paris, 1968, no. AO2192.
- 3) J.-P. Diard, P. Landaud, B. Le Gorrec, C. Montella, J. Electroanal. Chem., 255 (1988) 1.

Data files can be found in :

Fig. 1 :

C:\Users\xxx\Documents\EC-Lab\Data\Samples\Battery\AN42_battery

Fig. 5:

C:\Users\xxx\Documents\EC-Lab\Data\Samples\Corrosion\AN42_coating

APPENDIX

1) It is noteworthy that if the inductive loop in Fig. 5 could be fitted with an R/C instead of an R/Q (i.e. if a_2 was equal to 1) then an R+L would be enough and R+La unnecessary.

2) Furthermore, to widen the perception of what an equivalent circuit is, it is worth noting that $Z_Q(f) = Z_{La}(f)$ with $a_Q = -a_{La}$ and $Q = 1/La$, a_Q being the a parameter for the element Q and a_{La} for the element La.

If we replace in Eq. 4, a by $-a_Q$:

$$Z_{La}(f) = L_a (j2\pi f)^{-a_Q} \quad (5)$$

$$Z_{La}(f) = \frac{L_a}{(j2\pi f)^{a_Q}} \quad (6)$$

$$Z_{La}(f) = \frac{1}{Q(j2\pi f)^{a_Q}} \quad (7)$$

$$\text{With } L_a = \frac{1}{Q}$$

$$Z_{La}(f) = Z_Q(f) \quad (8)$$

Finally, the impedances of the C, L, Q and La elements are all particular forms of the general expression :

$$Z(f) = A(j2\pi f)^m \quad (9)$$

with A the value of the component and $m \in [-1,0[\cup]0,1]$.

If $m = 0$, then the impedance Z is a simple resistance.

Revised in 08/2019